
Residual concentration toward the boundary of the probe grid

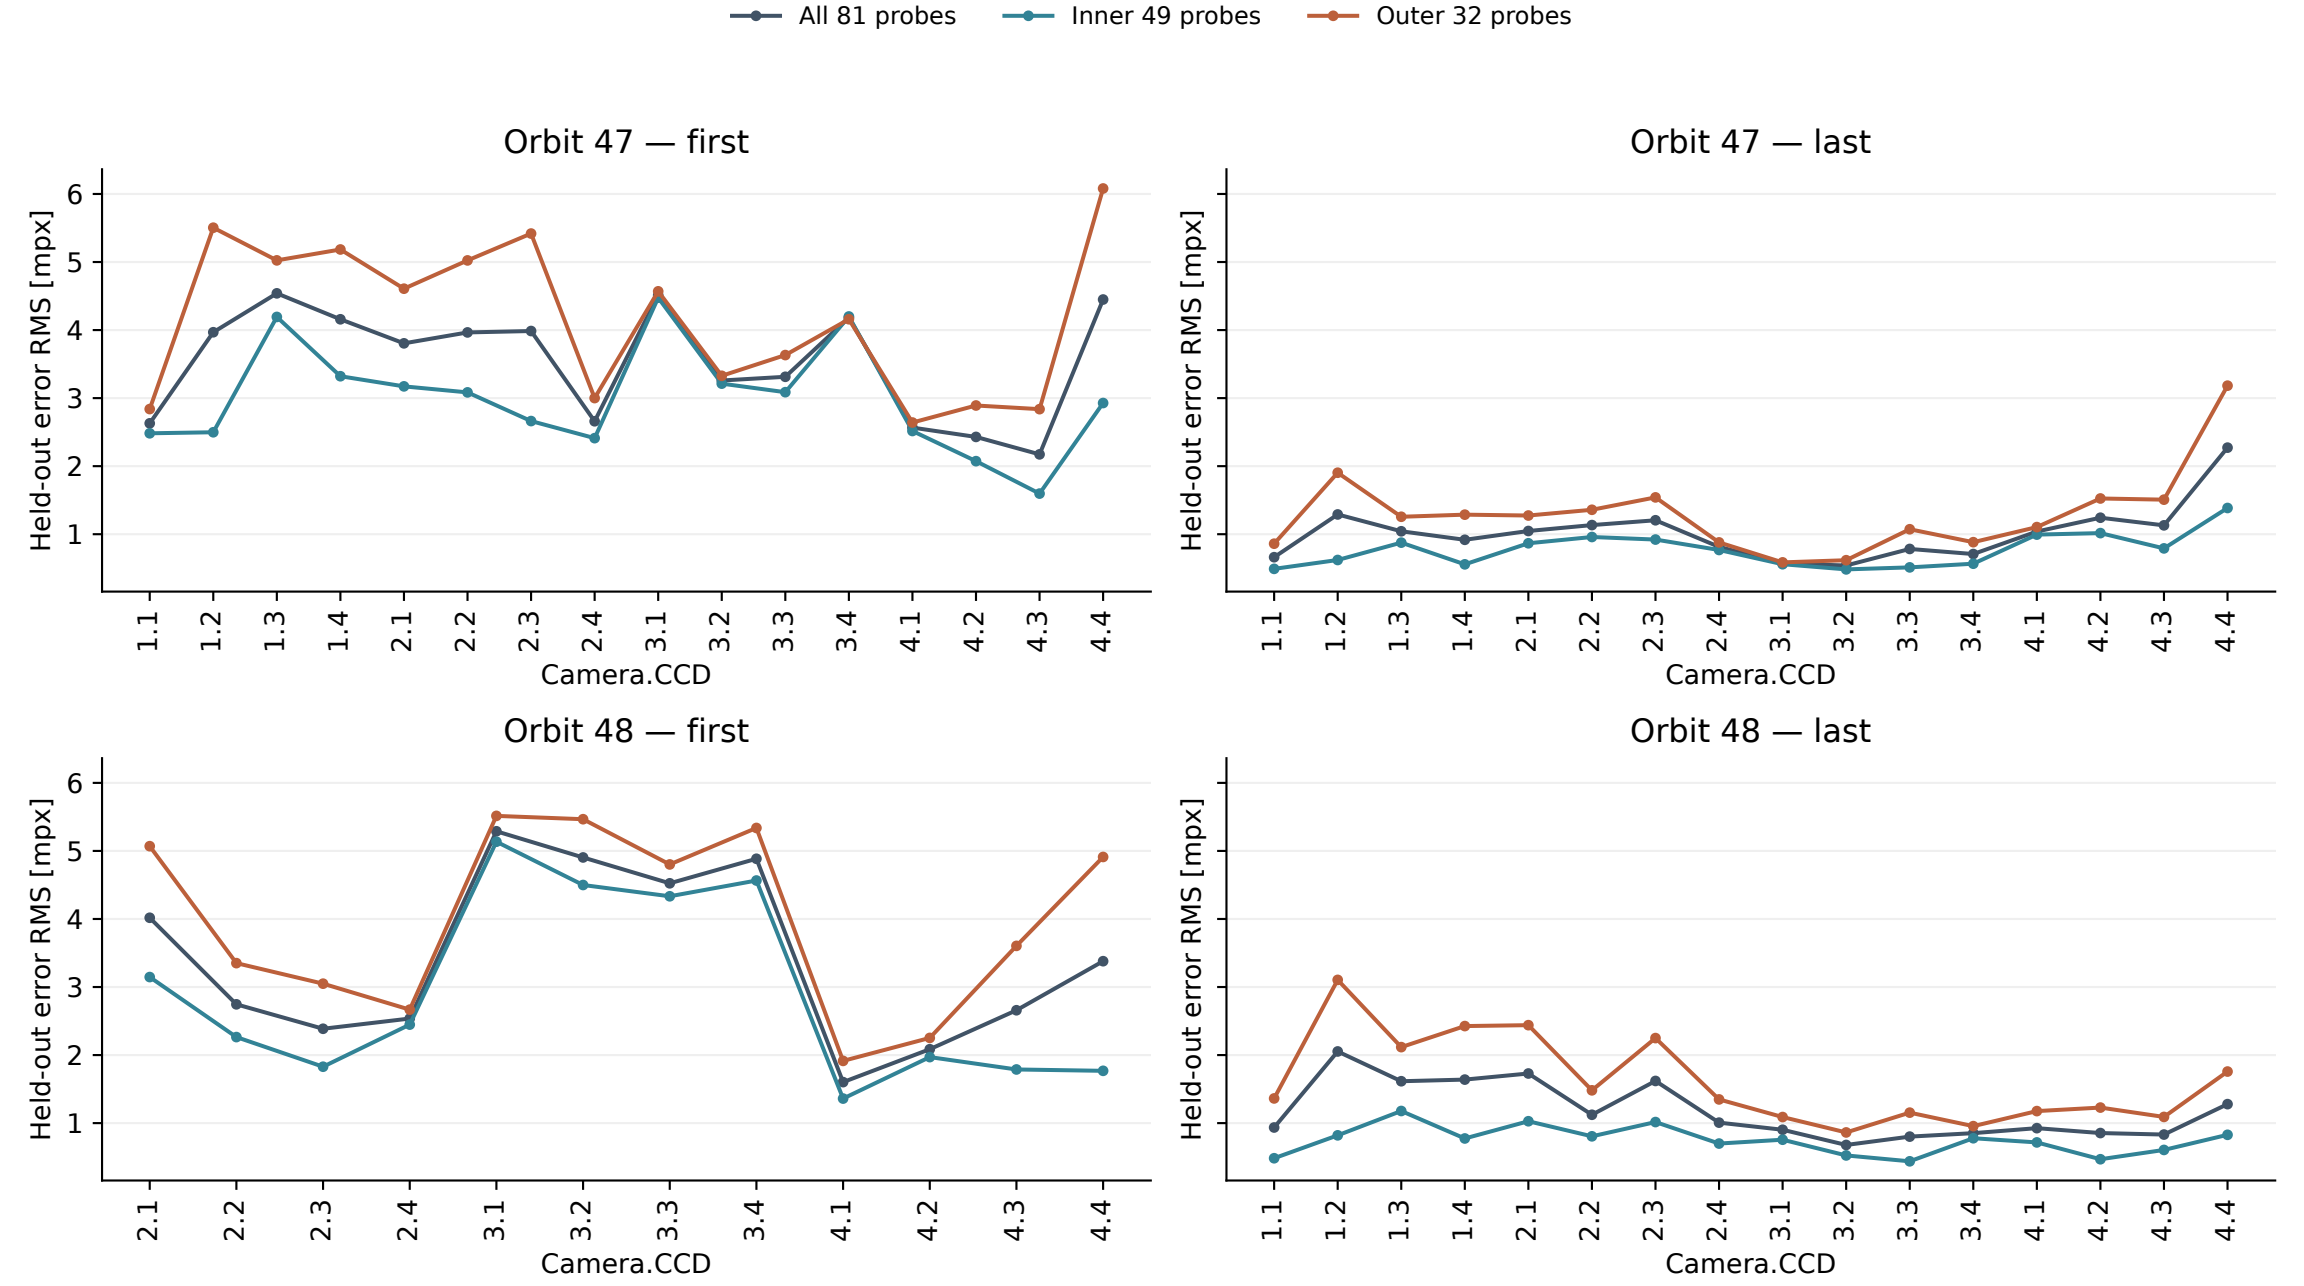

Descriptive support sensitivity only: predictions are unchanged; each RMS uses its stated probe denominator. The outer ring remains inset from detector edges.